



## Inserting your hearing aid batteries

Firstly, please note there are different Makes and Models of Hearing Instrument and correct battery Insertion will be a variation of one of the following themes:


Phonak Nathos Micro – Top View

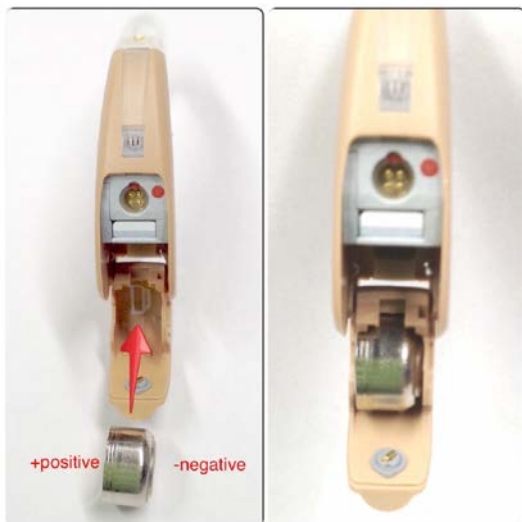

Phonak Nathos Micro – Side View

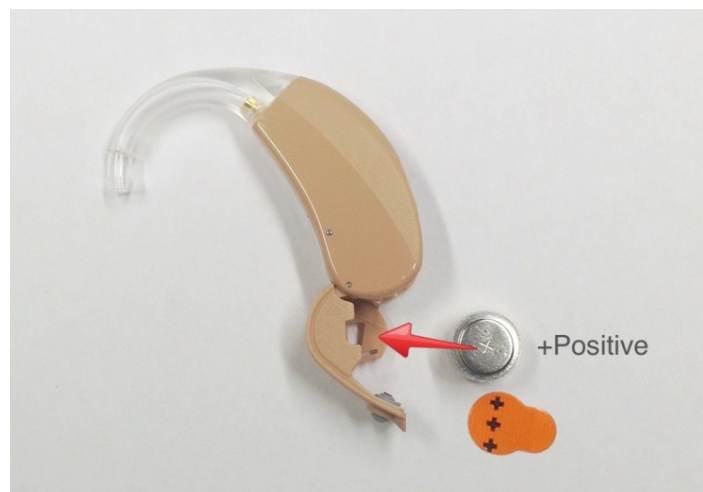


Phonak Nathos M / SP-W – Top View

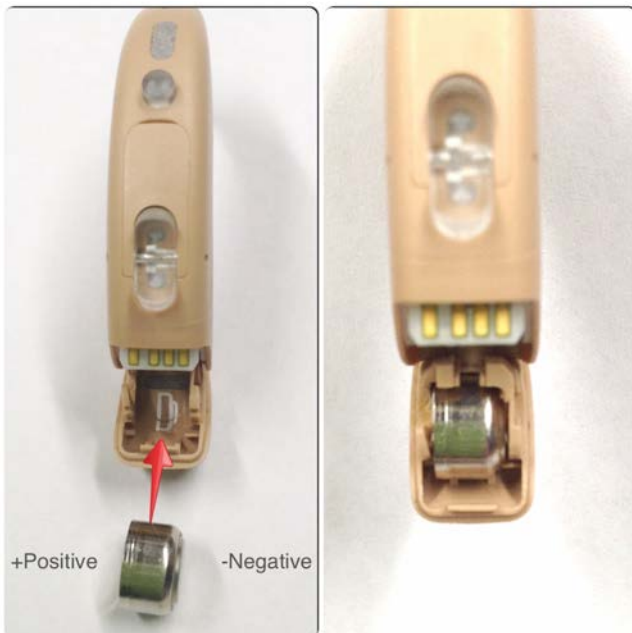


Phonak Nathos M / SP-W – Side View



Siemens Range ( M, DP, DSP ) – Side View

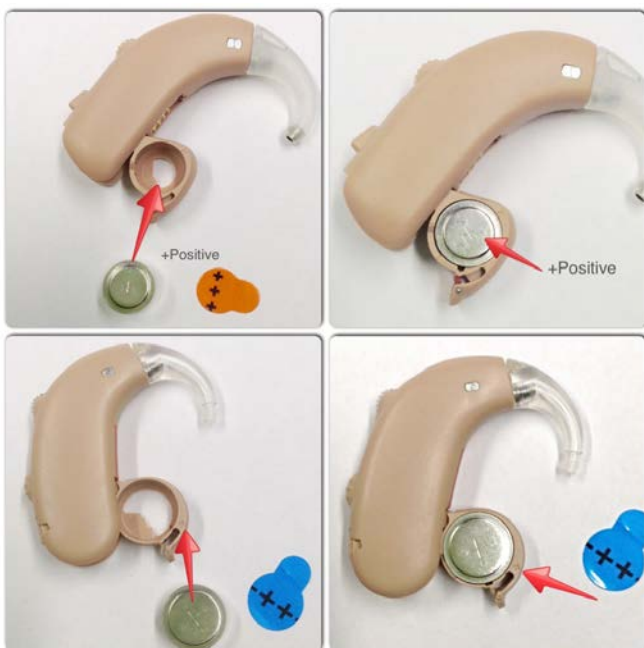

Phonak Nathos S+ Micro – Top & Side View

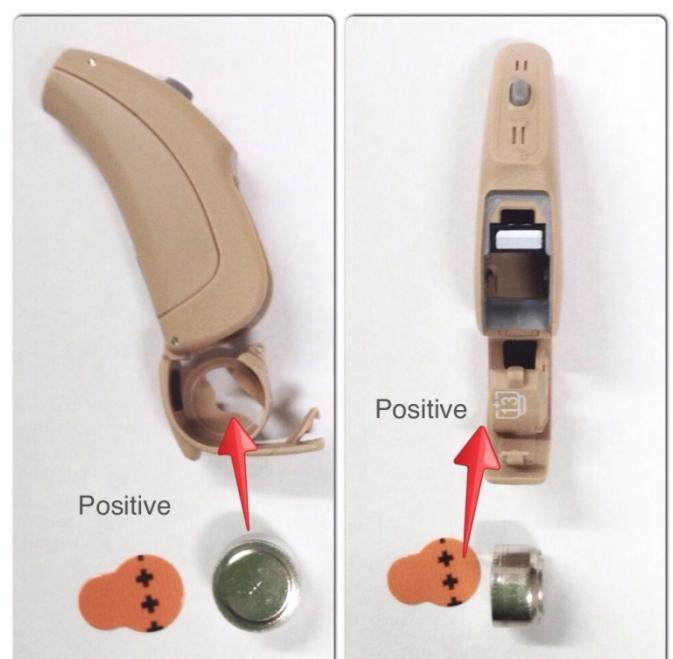

Phonak Nathos S+ M – Top & Side View

Phonak Nathos S+ UP-W – Top & Side View

